

CHAPTER 6

CONCLUSIONS AND FUTURE WORK

Chapter (6)

CONCLUSIONS AND FURTHER WORK

6.1. Conclusions

In the present study, the pump was tested in both direct (pump mode) and reverse (turbine mode) experimentally and numerically to investigate their performance for two sets of speeds of rotation. This study is widely applied in developing countries and rural areas, which is very significant solution for energy problems in Egypt.

The main starting points that can be drawn from the experimental results in this research:

- A pump could be operated as a turbine at different speeds of rotation without mechanical problems.
- An inline centrifugal pump which is considered a special type with low power could operate effectively as a turbine.
- An electronic load controller could control the operation of the turbine mode and fix the speed of rotation while the flow rate changes and could control the pump operation as well by adding batteries as a power source.

On the other hand, from the numerical results some conclusions are derived as:

- The flow through the inline pump could be simulated in pump mode and turbine mode.
- The shape of the volute casing has a great effect on the results at the pump mode.
- The numerical results are affected by the losses in the volute casing so the results have a difference with the experimental ones.

The comparison between the computational and experimental results shows good agreement at the turbine mode and shows a slight deviation at the pump mode.

6.2. Recommendations for future work

A parametric study should be conducted for the pump mode and turbine mode to study the effect of different parameters on the performance experimentally. These parameters are:

- The effect of impeller trimming on the performance of the pump and turbine modes.
- The effect of changing the outlet pipe geometry at the turbine mode.
- Adding two pumps in parallel and studying the effect of running two PATs in parallel instead of using a valve which dissipates energy to regulate the flow.
- Testing different inline pumps as turbines with different specific speeds and conclude correlations for each range of specific speed.

- Using a booster pump before the PAT at the turbine mode in order to test the pump at higher flow rates.

On the other hand, concerning the Numerical model a parametric study should be conducted for both modes to study the effect of different parameters on the performance. These parameters are:

- Using a dynamic mesh rather than the multiple frames of reference is more accurate as it eliminates the interpolation errors in the MRF approach.
- Changing the shape of the volute casing to obtain more optimum shape.
- Simulating the pump flow for more sets of rotational speeds.
- The internal losses and other modifications of the pump geometry (i.e. optimum shape) are to be studied which is difficult to measure experimentally.
- Effect of pump blade angle and number of the blades on the performance of turbine mode.

References

- 1- http://www.ksb.com/ksb-eg/Products_and_Services/Water/water_transport/PAT/657870/Pump-used-as-turbine.html (access on 15/2/2014).
- 2- Chapallaz J. M., Eichenberger P. and Fischer G., “Manual on Pumps Used as Turbines”, MHPG Series “Harnessing Water Power on a Small Scale”, Volume 11., 1992.
- 3- Pool D., “Investigating a Buoy Pump System for The Electrolysis of Seawater into Potable Water”, Internal Report, Renewable energy department, Oregon Institute Of Technology, December 2012.
- 4- <http://www.eurelectric.org/water> (access on 30/10/2014).
- 5- Alatorre-Frenk C., “Cost Minimisation in Micro-Hydro Systems Using Pumps-As-Turbines”, University of Warwick, 1994.
- 6- Garay P. N., “Using Pumps as Hydroturbines”, Hydro Review, 1990.
- 7- <http://www.waterworld.com/articles/print/volume-27/issue-2/departments/pump-tips-techniques/case-history-pumps-as-turbines-in-the-water-industry.html> (access on 18/3/2014)
- 8- Williams A. A., “Pumps as Turbines: A User's Guide”, Intermediate Technology Publications, 1995.
- 9- Heng S. S., ”Design of a 5 Kw Microhydro Generating Set”, University of Canterbury, 1992.
- 10- Boothe P. M. and Lewis C. K., “The operation of centrifugal pumps under abnormal conditions”, M.Sc., California Institute of Technology, California, 1932.
- 11- Maher P., Smith N. P. A., Williams A.A., “Assessment of pico hydro as an option for off-grid electrification in Kenya”, The Nottingham Trent University, Nottingham, Renewable Energy Vol. 28, PP. 1357–1369, Elsevier, 2002.
- 12- Nautiyal H. , Varun and Kumarn A., “Reverse running pumps analytical, experimental and computational study: A review”, National Institute of Technology, Hamirpur, India, Renewable and Sustainable Energy Reviews Vol. (14), PP. 2059–2067, 2010.

- 13- Motwania K. H., Jain S. V., Patel R. N., “Cost analysis of pump as turbine for pico hydropower plants – a case Study”, Institute of Technology, Nirma university, India, Procedia Engineering Vol. (51), PP. 721 – 726, 2013.

- 14- Smith N.P.A., Williams A. A., Harvey A. B., Waltham M. and Nakarmi A-M, “Direct Coupled Turbine-Induction Generator Systems for Low-cost Micro-hydro Power”, 2nd World Renewable Energy Congress "Renewable Energy Technology and the Environment" (Reading, UK), Pergamon, Vol. (5), PP. 2509-16, 1992.

- 15- Williams A.A., “Pumps as Turbines Used with Induction Generators for Stand-alone Micro-hydroelectric Power Plants”, PhD thesis, Nottingham-Trent University, 1992.

- 16- Nepal Micro Hydro Power, “Pump-As-Turbine Technology”, Intermediate Technology Development Group, 2005, www.microhydro.org.np .

- 17- Derakhshan S. and Nourbakhsh A. “Experimental study of characteristic curves of centrifugal pumps working as turbines in different specific speeds”, Experimental Thermal and Fluid Science Vol. (32), PP. 800–807, Elsevier ,2007.

- 18- Stepanoff A. J., “Centrifugal and Axial Flow Pumps, Design and Applications”, 2nd edition, John Wiley and Sons, Inc., New York,1957.

- 19- Gopalakrishnan S., “Power Recovery Turbines for the Process Industry”, 3rd International Pump Symposium (Houston), Texas A & M University, PP. 3-11, 1986.

- 20- Miller R. W., “Flow Measurement Engineering Handbook”, Third edition, McGRAW-Hill, 1996.

- 21- Childs P. R. N.,”Rotating Flow”, Elsevier, 2011.

- 22- FLUENT documentation. (2009). USA: Fluent Inc.

- 23- Shih T. H., Liou W. W., Shabbir A., Yang Z. and Zhu J. A, “New k-epsilon Eddy- Viscosity Model for High Reynyolds Number Turbulent Flows - Model Development and Validation.” Computer Fluids, Vol. 24, 227-238., 1995.

- 24- Reynolds O., “On the Dynamical Theory of Incompressible Viscous Fluids and the Determination of the Criterion. Philosophical Transactions of the Royal Society”, Vol. 186, PP. 123-164, 1895.

25- Zadavec M., Basic S., Hribersek M., “The Influence Of Rotating Domain Size In A Rotating Frame Of Reference Approach For Simulation Of Rotating Impeller In A Mixing Vessel”, Journal Of Engineering Science And Technology, Vol. 2, No. 2, 2007.

26- Miller R., “Flow Measurement Engineering Handbook”, 3rd edition, McGRAW-Hill, 1996.

Appendix (A)

Pressure gauges calibration

The upstream and downstream pressure gauges used in the experimental setup were calibrated in the fluid mechanics laboratory using a pneumatic pressure tester (DRUCK- DPI 610). The calibration curves are as follows:


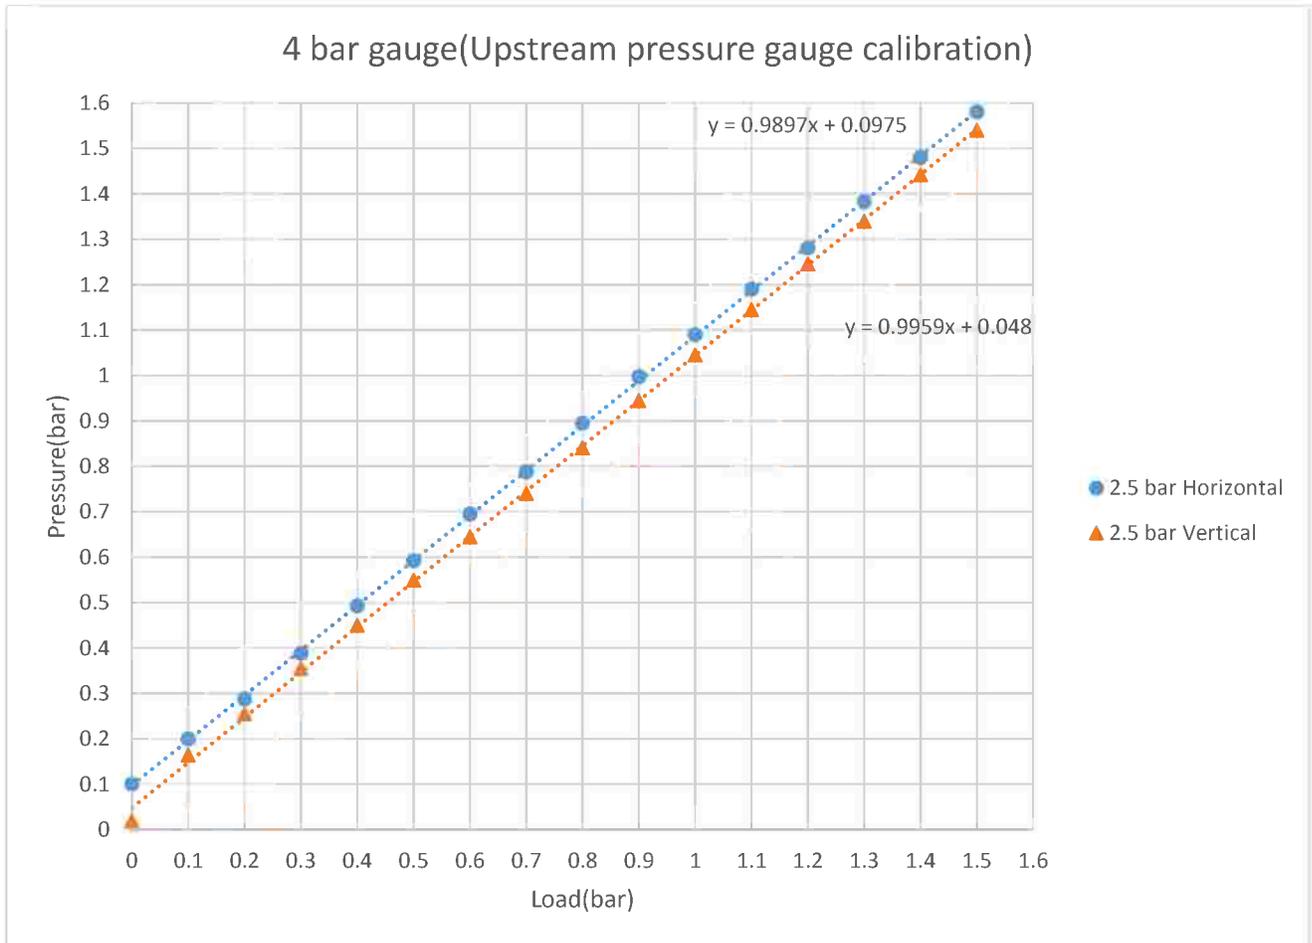


Figure (A-1) Pressure gauge calibration (4 bar)

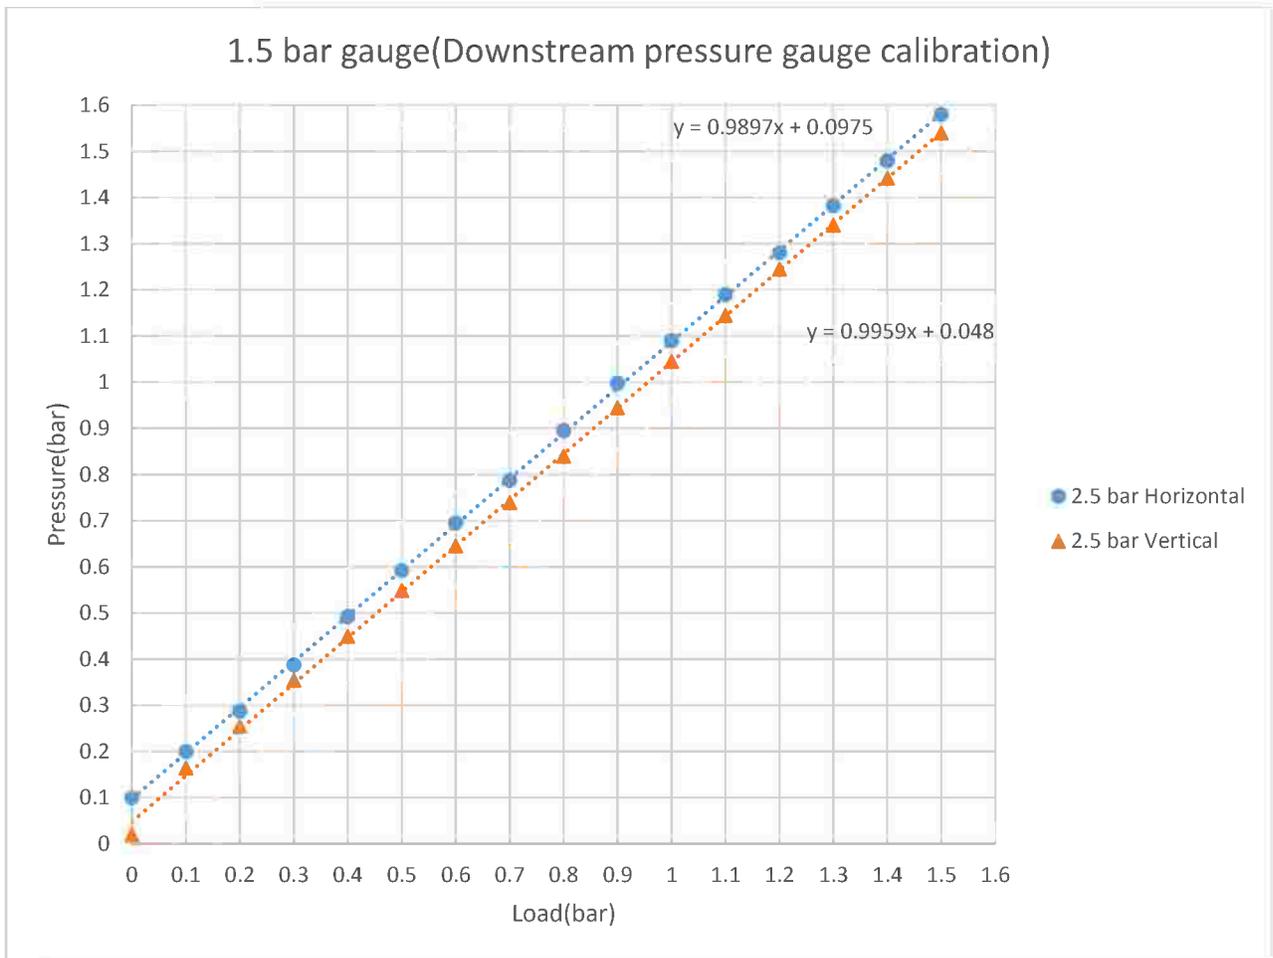

Figure(A-2) pressure gauge calibration (1.5 bar)

Orifice calibration:

The orifice meter was calibrated in the Fluid mechanics laboratory. A tank of volume 26.719 liter was used in the calibration process.

The Foxboro Integral Orifice Flow Meter Assembly (IFOA) and the honed-orifice meter run are widely used in line sizes of ½ to 1 ½. They have corner taps, since flange or D and D/2 taps would be located in regions where pipe friction would influence the differential [26].

$$C = C_{\infty} + b/R_D^n$$

Where C_{∞} is a factor which could be estimated from the following equation:

$$C_{\infty} = a + b * \beta^{2.1} + c * \beta^8 + d * \frac{\beta^4}{1 - \beta^4} + e * \beta^3$$

Coefficient b could be estimated from the following equation:

$$b = f + g * \beta + h * \beta^2 + i * \beta^3 + j * \beta^4$$

Integral flow orifice assembly IFOA

Square-edged D=1in

$$C_{\infty} = 0.6050 - 0.1837 * \beta^2 + 0.6615 * \beta^4 - 1.094 * \beta^8$$

Coefficient b equation

$$b = 1.646 * \beta^{0.5} + 2.394 * \beta^{\frac{5}{2}} - 4.899 * \beta^{\frac{9}{2}}$$

Exponent n=0.5

Recommended accuracy and restrictions for equations

Honed meter runs

Nominal pipe dia. D (in)	Beta Ratio β	Pipe Re R_D	Coefficient accuracy %
½ - 1½	0.1-0.8	>1000	±0.75

Integral flow orifice assembly IFOA (Foxboro)

Nominal pipe dia. D (in)	Beta Ratio β	Pipe Re R_D	Coefficient accuracy %
	STD sizes	$1500/\beta \leq R_D/\beta$	±0.75

Plate thickness = 0.125 in for D<6 in (D*<150mm) & 0.2< β <0.75

C from the theoretical calculations is 0.67576 while it is 0.754 from the experimental results. This difference is due to the special design of the corner taps.

The relation between the velocity and C_D is plotted using calibration results. In addition, the relation between the Re and C_D based on bore diameter is plotted. The trend of both curves is similar to the real ones.

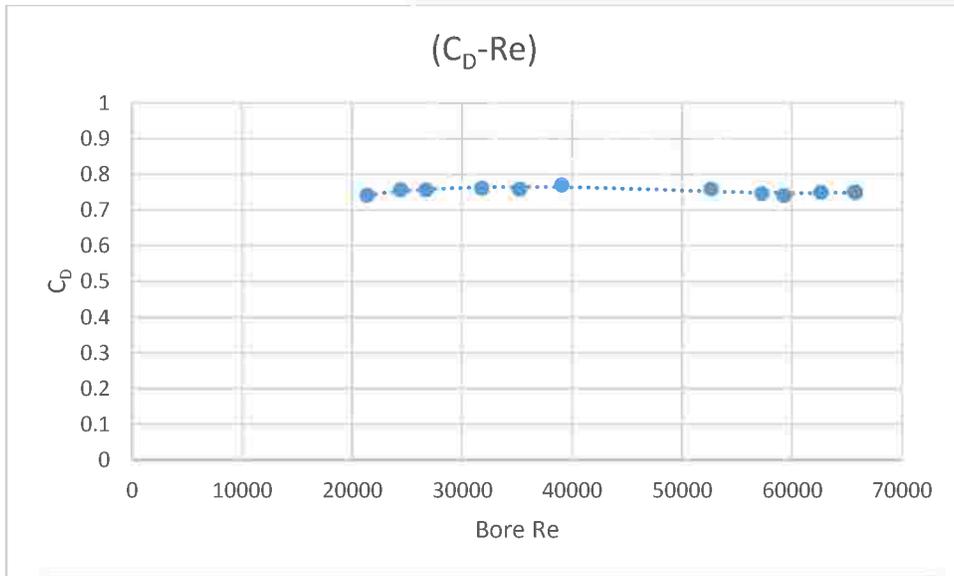


Figure (A-3) Calculated curve of orifice meter (Variation of orifice coefficient of discharge C_D with Reynolds number Re (based on orifice diameter))

Appendix (B)

Repeatability test

The repeatability of the results were tested in different speeds of rotation of the DC motor at the Fluid mechanics laboratory. The repeatability results are shown in Figures(B-1 to B-7)

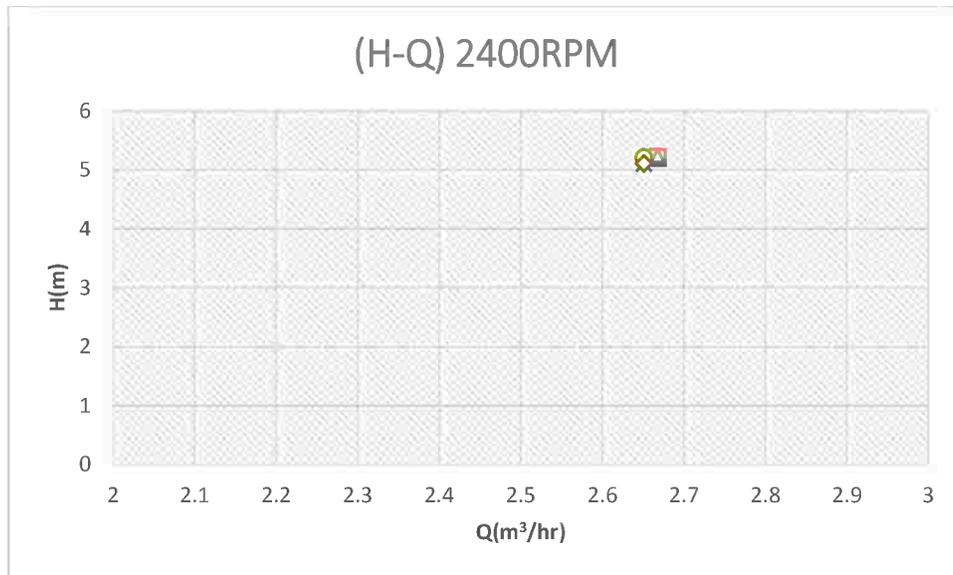


Figure (B-1) Repeatability test at 2400RPM

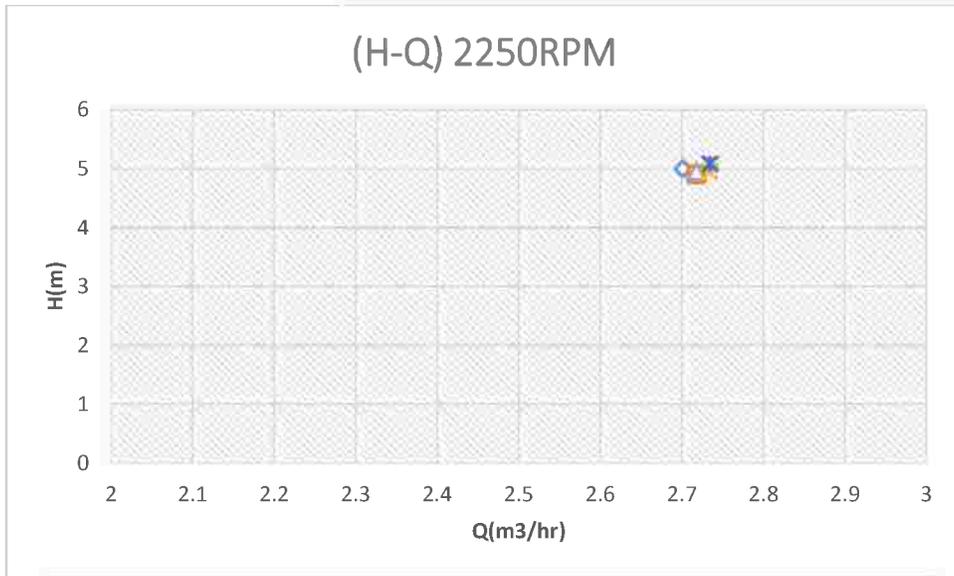


Figure (B-2) Repeatability test at 2250RPM

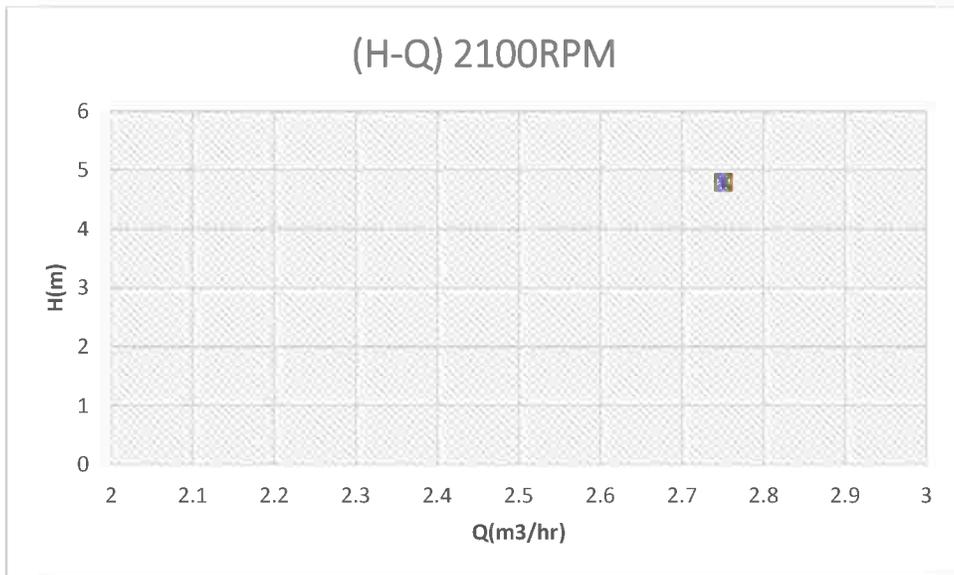


Figure (B-3) Repeatability test at 2100RPM

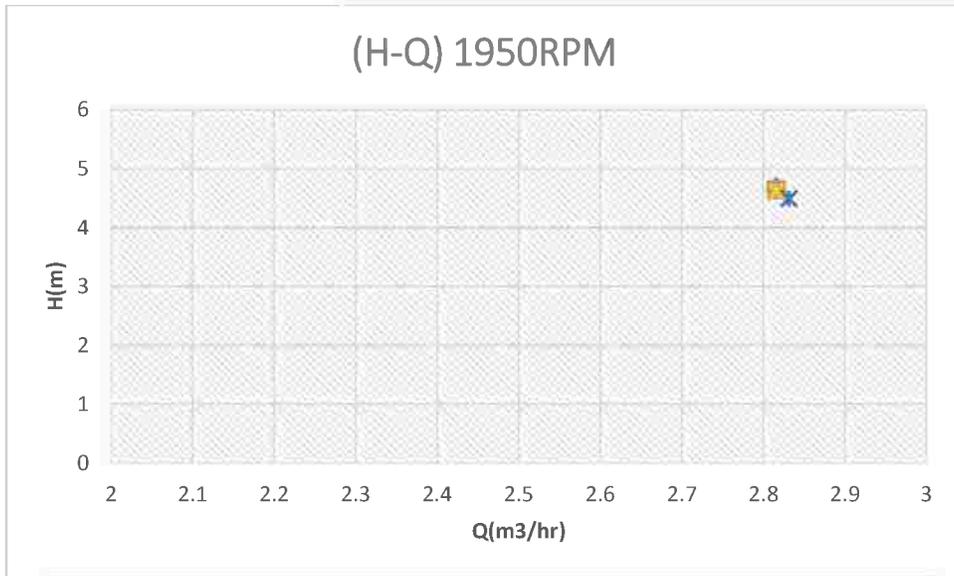


Figure (B-4) Repeatability test at 1950RPM

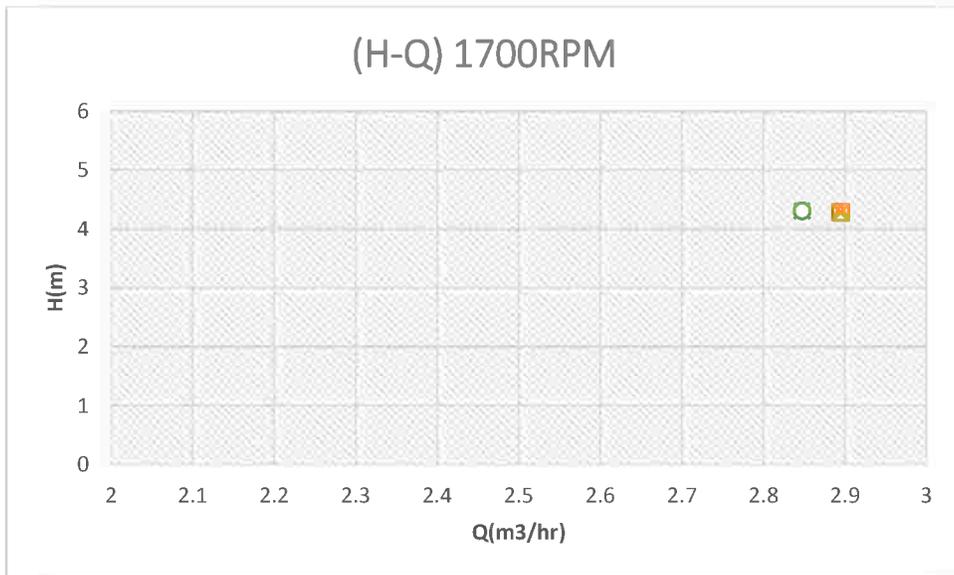


Figure (B-5) Repeatability test at 1700RPM

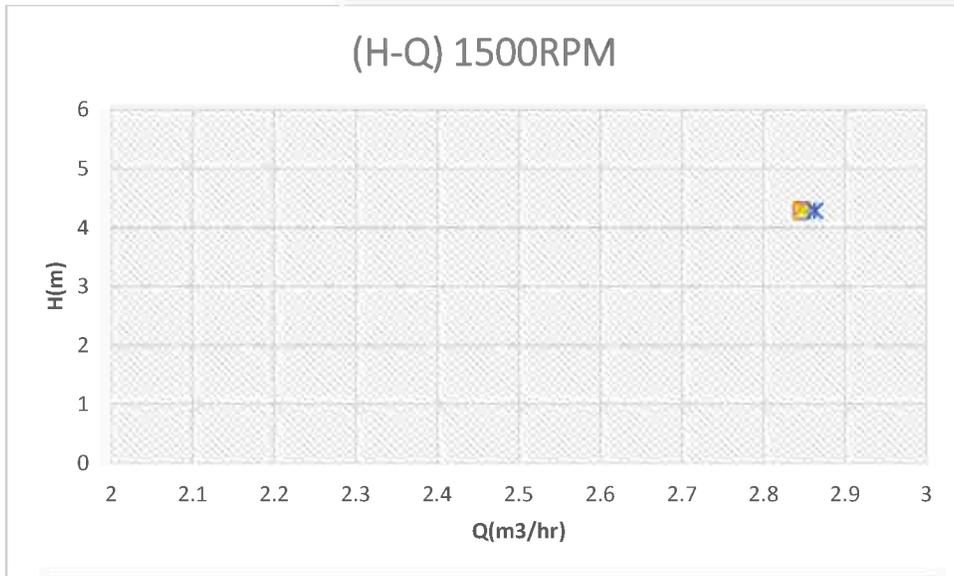


Figure (B-6) Repeatability test at 1500RPM

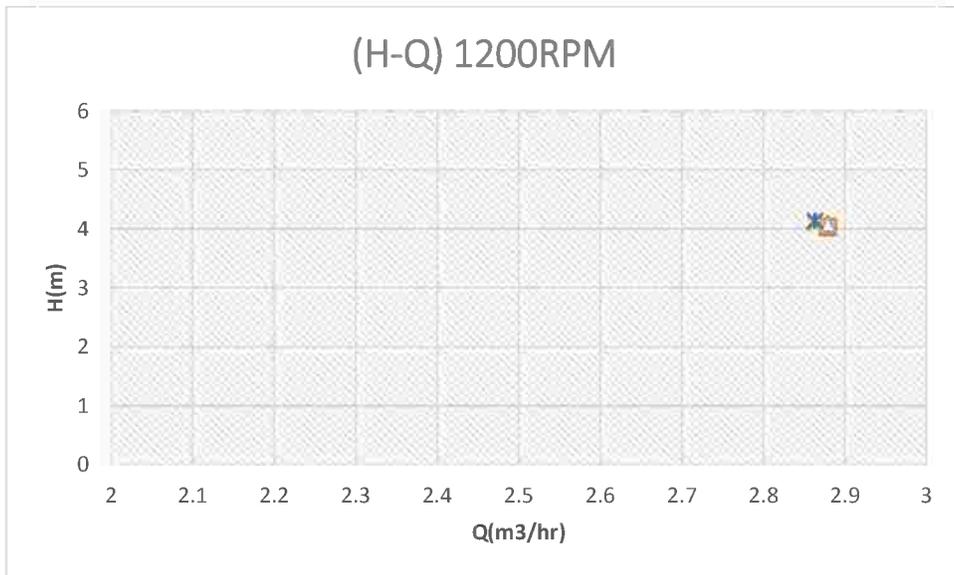


Figure (B-7) Repeatability test at 1200RPM

Uncertainty analysis:

Uncertainty analysis of volume flow rate

The volume flow rate passing through the orifice meter is a function of the U-tube manometer differential pressure reading, y , which is related to the pressure head, h , as follows:

$$Q = c_d a_o \sqrt{2gh}$$

$$\text{Where } h = y \left(\frac{S.G_u}{S.G_f} - 1 \right)$$

Where c_d is the discharge coefficient which is calibrated experimentally to be 0.754, a_o is the bore diameter of the orifice, $S.G_u$ and $S.G_f$ are the specific gravity of the differential fluid and the fluid flowing through the pipe respectively.

As a result, the uncertainty of the volume flow rate depends on the uncertainty of the differential pressure reading of the manometer. Therefore, the uncertainty of the differential pressure reading or the deviation could be calculated using calculus as the deviation in Q which is a single-variable function $Q(y)$, the deviation in Q can be related to the deviation in y using calculus as follows:

$$\delta_Q = \left(\frac{dQ}{dy} \right) \delta_y$$

Thus, taking the square and the average:

$$\delta_Q^2 = \left(\frac{dQ}{dy} \right)^2 \delta_y^2$$

And using the definition of σ , the standard error, we get:

$$\sigma_Q = \left| \frac{dQ}{dy} \right| \sigma_y$$

By applying these equations on the flow rate:

$$\frac{dQ}{dy} = \text{const.} * \frac{1}{\sqrt{y}}$$

$$\text{Where } \text{const.} = \frac{c_d a_o \sqrt{2g}}{2} = 0.001471044$$

$$\sigma_Q = \text{const.} * \frac{1}{\sqrt{y}} * \sigma_y$$

In order to calculate σ_y for N measurements rules of measuring the uncertainty in repeated measurements are applied as follows:

1. Sum all the measurements and divide by 5 to get the average or mean:

$$y_{\text{avg}} = \frac{0.092 + 0.092 + 0.092 + 0.091 + 0.091}{5} = 0.0916 \text{ m}$$

2. Now, subtract this average from each of the 5 measurements to obtain 5 "deviations":

$$y_1 - y_{\text{avg}} = 0.0004$$

$$y_2 - y_{\text{avg}} = 0.0004$$

$$y_3 - y_{\text{avg}} = 0.0004$$

$$y_4 - y_{\text{avg}} = -0.0006$$

$$y_5 - y_{\text{avg}} = -0.0006$$

3. Square each of these 5 deviations and add them all up and divide the result by (N-1), and then take the square root to obtain the standard deviation, s,

$$s = \sqrt{\frac{0.0004^2 + 0.0004^2 + 0.0004^2 + 0.0006^2 + 0.0006^2}{4}} = 0.000547723$$

$$\sigma_y = \frac{s}{\sqrt{N}} = 0.000244949$$

$$\therefore \sigma_Q = \frac{0.001471044}{\sqrt{0.0916}} * 0.000244949 = 1.19057\text{E-}06 \text{ m}^3/\text{s} = 0.004286 \text{ m}^3/\text{hr}$$

$$\therefore Q = Q_{\text{avg}} \pm \sigma_Q$$

Where

$$Q_{\text{avg}} = \frac{2.87909 + 2.879091 + 2.879091 + 2.863401 + 2.86340108}{5} = 2.879091 \text{ m}^3/\text{hr}$$

$$\therefore Q = 2.879091 \pm 0.004286 \text{ m}^3/\text{Hr}$$

So the uncertainty of the flowrate measurement is $\pm 0.4286\%$

Uncertainty analysis of pressure

The uncertainty of the pressure is easily calculated as it is not a function of any variable. The same steps of getting σ_y is applied.

$$\therefore \Delta p = \Delta p_{\text{avg}} \pm \sigma_p$$

$$\therefore \Delta p = 0.399 \pm 0.001870829 \text{ bar}$$

So the uncertainty of the pressure measurement is $\pm 0.187\%$

Uncertainty analysis of power

The power is a function of two variables: the volt and the current.

In the case where P depends on two or more variables, the derivation above can be repeated with minor modification. For two variables, P(V, I), we have:

$$\delta P = \left(\frac{\partial P}{\partial V}\right) \delta V + \left(\frac{\partial P}{\partial I}\right) \delta I$$

Thus taking the square and the average, we get the **law of propagation of uncertainty**:

$$(\delta P)^2 = \left(\frac{\partial P}{\partial V}\right)^2 (\delta V)^2 + \left(\frac{\partial P}{\partial I}\right)^2 (\delta I)^2 + 2 \left(\frac{\partial P}{\partial V}\right) \left(\frac{\partial P}{\partial I}\right) \delta V \delta I$$

If the measurements of x and y are uncorrelated, then $\delta V \delta I = 0$ and using the definition of σ_p , we get:

$$\sigma_p = \sqrt{\left(\frac{\partial P}{\partial V}\right)^2 \sigma_V^2 + \left(\frac{\partial P}{\partial I}\right)^2 \sigma_I^2}$$

$$\frac{\partial P}{\partial V} = I, \quad \frac{\partial P}{\partial I} = V$$

$$\therefore \sigma_p = \sqrt{I^2 \sigma_V^2 + V^2 \sigma_I^2}$$

$$\therefore \sigma_p = \sqrt{0.432^2 * 0.04^2 + 11.34^2 * 0.002^2} = 0.0285$$

$$\therefore \text{Power} = 4.899 \pm 0.0285 \text{ watt}$$

So the uncertainty of the power measurement is $\pm 2.85\%$

APPENDIX (C)

Arduino Code of the electrical circuit

```
int sensorPin = A1; // select the input pin for the potentiometer
int ledPin = 13; // select the pin for the LED
int sensorValue = 0; // variable to store the value coming from the sensor
int pwm=9;
void setup() {
  // declare the ledPin as an OUTPUT:
  pinMode(ledPin, OUTPUT);

}

void loop() {
  setPwmFrequency(pwm, 128);
  // read the value from the sensor:
  sensorValue = analogRead(sensorPin);
  sensorValue=sensorValue/4.0;
  analogWrite(sensorValue, pwm);
  TCCR2B = TCCR2B & 0b11111000 | mode;
}
}

void setPwmFrequency(int pin, int divisor) {
  byte mode;
  if(pin == 5 || pin == 6 || pin == 9 || pin == 10) {
    switch(divisor) {
```

```

case 1: mode = 0x01; break;

case 8: mode = 0x02; break;

case 64: mode = 0x03; break;

case 256: mode = 0x04; break;

case 1024: mode = 0x05; break;

default: return;

}

if(pin == 5 || pin == 6) {
    TCCR0B = TCCR0B & 0b11111000 | mode;
} else {
    TCCR1B = TCCR1B & 0b11111000 | mode;
}

} else if(pin == 3 || pin == 11) {
switch(divisor) {
    case 1: mode = 0x01; break;

    case 8: mode = 0x02; break;

    case 32: mode = 0x03; break;

    case 64: mode = 0x04; break;

    case 128: mode = 0x05; break;

    case 256: mode = 0x06; break;

    case 1024: mode = 0x07; break;

    default: return;

}

```

ملخص الرسالة

نظرا لزيادة التطبيقات في استخدام المضخات كتوربينات، فإنه من الضروري أن نحصل على معلومات عملية حقيقية تتعلق بهذا الموضوع. الهدف من هذه الرسالة هو تمثيل مضخة الطرد المركزي ذات المحور الواحد كتوربينة عمليا و حسابيا و دراسة العلاقة بين منحنيات الأداء لهما.

الجهاز العملي مكون من مضخة طرد مركزي متصلة مباشرة بمحرك كهربى ذو تيار مباشر. أداء المضخة في الوضع المباشر يتم اختبارها عن طريق التحكم في فتحة صمام الخروج حتى نحصل على منحنى الأداء. المحرك كهربى ذو التيار المباشر يتم التحكم فيه عن طريق دائرة كهربية للتحكم في سرعة دورانه. علاوة على ذلك، فإن المضخة يتم اختبارها في الوضع المعاكس كتوربينة عن طريق التحكم في صمام الخروج السابق ذكره للحصول على منحنيات الأداء لنفس سرعات الدوران للوضع المباشر. من هنا، العلاقة بين منحنيات الأداء يتم تعريفها بوضوح.

السريان خلال المضخة يتم استنتاجه عن طريق ديناميكا الموائع الحسابية باستخدام برنامج "Fluent" و النتائج تم اختبارها و التحقق من صحتها باستخدام النتائج العملية. النموذج العددي تم استخدامه للتنبؤ بمنحنيات الأداء للمضخة و التوربينة عند سرعات دوران مختلفة عن السرعات العملية.

و في هذه الرسالة تم التنبؤ بالنتائج النظرية و التحقق م صحتها باستخدام النتائج العملية و التي أثبتت أن النتائج تتوافق في سلوك التغيير و يوجد فرق بين القيم العملية و النظرية تحتاج إلى دراسات مستقبلية لتقليل الفروق.

و قد توصلت الدراسة إلى:

- إمكانية استخدام المضخات ذات الطرد المركزي في عملية توليد الطاقة الكهرومائية الصغيرة المقدار بطريقة سريعة و رخيصة.
- إمكانية استخدام ميكانيكا الموائع العددية في التنبؤ بأداء المضخة الطاردة المركزية ذات الخط الواحد عندما تعمل كمضخة أو توربين حيث يمكن اختيار المضخة المناسبة في الموقع المناسب إذا علم كمية التصرف و الرافع الخاص بالطاقة المائية المتاحة.



كلية الهندسة
جامعة الإسكندرية
قسم الهندسة الميكانيكية

دراسة استخدام مضخات الطرد المركزي ذات الخط الواحد كتوربينات

مقدمة إلى قسم الهندسة الميكانيكية

كلية الهندسة – جامعة الإسكندرية

ضمن متطلبات الحصول على درجة

الماجستير في الهندسة الميكانيكية

آية صادق زكريا كساب

2014

لجنة الإشراف:

أ.د/ مدحت عباس شوقي

قسم الهندسة الميكانيكية - جامعة الإسكندرية

د/ إيهاب جابر آدم

قسم الهندسة الميكانيكية - جامعة الإسكندرية

التوقيع بالموافقة:

.....

.....

دراسة استخدام مضخات الطرد المركزي ذات الخط الواحد كتوربينات

مقدمة من المهندسة

آية صادق كساب

للحصول على درجة

ماجستير العلوم الهندسية

في

الهندسة الميكانيكية

التوقيع بالموافقة:

.....

.....

.....

لجنة المناقشة و الحكم على الرسالة:

أ.د/ محمد فريد خليل

قسم الهندسة الميكانيكية - جامعة الإسكندرية

أ.د/ مدحت عباس شوقي

قسم الهندسة الميكانيكية - جامعة الإسكندرية

أ.د/ مصطفى نصر محمد نصر

قسم هندسة القوى الميكانيكية بشبين الكوم – جامعة المنوفية

.....

أ.د / هبة وائل لهيطة

وكيل الكلية لشئون الدراسات العليا و البحوث
كلية الهندسة - جامعة الإسكندرية